This document contains symbols that may appear on Axis Spine Technologies product packaging or labeling. It provides information on the symbol including the standards title, reference, and description, where available.

Please read the full Instructions for Use for detailed information on proper use, indications, contraindications, warnings, precautions and adverse events. This document does not replace the Instructions for Use.

Table 1 – Symbols derived from ISO 15223-1. Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied.

Symbol	Symbol Title	Explanatory Text
	Manufacturer.	Indicates the medical device manufacturer.
	Date of manufacture.	Indicates the date when the medical device was manufactured.
	Use by.	Indicates the date after which the medical device is not to be used.

Symbol	Symbol Title	Explanatory Text
	Batch code.	Indicates the manufacturer's batch code so that the batch or lot can be identified.
	Catalogue number.	Indicates the manufacturer’s catalogue number so that the medical device can be identified.
	Distributor.	Indicates the entity distributing the medical device into the locale.
	Country of manufacture.	To identify the country of manufacture of products.
	Sterile.	Indicates a medical device that has been subjected to a sterilization process.
	Sterilized using irradiation.	Indicates a medical device that has been sterilized using irradiation.
	Sterilized using steam or dry heat.	Indicates a medical device that has been sterilized using steam or dry heat.

Symbol	Symbol Title	Explanatory Text
	Do not resterilize.	Indicates a medical device that is not to be resterilized.
	Non-sterile.	Indicates a medical device that has not been subjected to a sterilization process.
	Do not use if package is damaged and consult instructions for use.	Indicates that a medical device that should not be used if the package has been damaged or opened and that the user should consult the instructions for use for additional information.
	Single sterile barrier system.	Indicates a single sterile barrier system.
	Single sterile barrier system with protective packaging inside.	Indicates a single sterile barrier system with protective packaging inside.

Symbol	Symbol Title	Explanatory Text
	Keep dry.	Indicates a medical device that needs to be protected from moisture.
	Do not reuse.	Indicates a medical device that is intended for one single use, or for use on a single patient during a single procedure.
	Consult instructions for use or consult electronic instructions for use.	Indicates the need for the user to consult the instructions for use.
	Caution.	Indicates that caution is necessary when operating the device or control close to where the symbol is placed, or that the current situation needs operator awareness or operator action in order to avoid undesirable consequences.
	Patient number.	Indicates a unique number associated with an individual patient.

Symbol	Symbol Title	Explanatory Text
	Patient name.	Indicates the name of the patient.
	Patient identification.	Indicates the identification data of the patient.
	Patient information website	Indicates a website where a patient can obtain additional information on the medical product.
	Health care center or doctor.	Indicates the address of the health care center or doctor where medical information about the patient may be found.
	Date.	Indicates the date that information was entered or a medical procedure took place.

Symbol	Symbol Title	Explanatory Text
	Medical device.	Indicates the item is a medical device.
	Unique device identifier.	Indicates a carrier that contains unique device identifier information.

Table 2 – Symbols derived from Title 21 Code of Federal Regulations Parts 801.109

Symbol	Symbol Title	Explanatory Text
	Prescription only.	Caution: Federal law restricts this device to sale by or on the order of a license healthcare practitioner.

Table 3 – Symbols derived from ISO 7001 - Graphical Symbols for Use on Equipment

Symbol	Symbol Title	Explanatory Text
	General mandatory action sign.	To signify a mandatory action.
	Lock.	Indicates a mechanism that is locked when moved to this configuration.
	Unlock.	Indicates a mechanism that is unlocked when moved to this configuration. **Note** – This symbol may be mirrored on Axis product.

Table 4 – Non-Standard Symbols

Symbol	Symbol Title	Explanatory Text
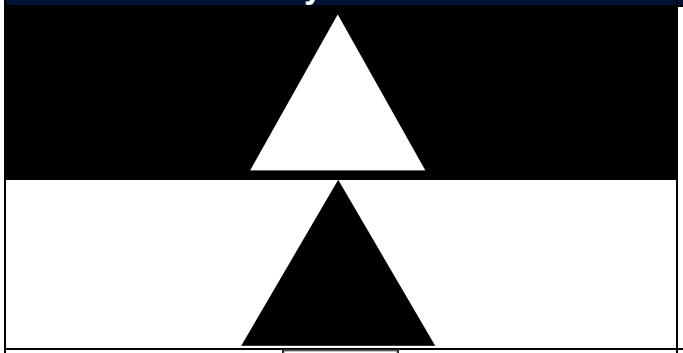	Revision.	An internal identifier to denote the revision of a medical device.
	Global Trade Item Number.	Symbol denoting global trade item number. This serves as an indicator for the unique identifier for the product.
	Axis Logo.	Logo used to denote Axis products.
	Endplate – Inferior.	Indicates instrument must be used with an Inferior Endplate.

Symbol	Symbol Title	Explanatory Text
	Endplate – Superior.	Indicates instrument must be used with a Superior Endplate.
	Disassemble before cleaning.	Components must be disassembled prior to undergoing a cleaning and sterilization cycle.
	Do not disassemble.	Indicates the instrument should not be disassembled.
	Lubricate.	Indicates lubrication is required.